

April 16, 2018


▪ **TEST REPORT** ▪

**PN 140575**


**CHEMICAL ANALYTICAL SERVICES**

Todd Zuella  
**SAS Safety Corporation**  
3031 Gardenia Avenue  
Long Beach, CA 90807

Prepared By:

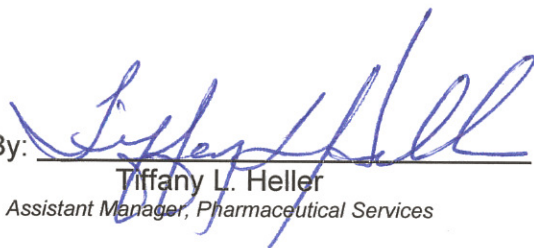  
Tiffany L. Heller  
Assistant Manager, Pharmaceutical Services

Approved By:

  
Ana C. Barbur, M.S.  
Vice President, Analytical & Chemical Services



\*Certificate Numbers 255.01 & 255.02

An A2LA Accredited Testing Laboratory — Certificate Numbers 255.01 & 255.02  
ISO 9001:2008 Registered

**ISO 9001:2008**  
Registered

Letters and reports are for the exclusive use of the clients to whom they are addressed and shall not be reproduced, except in full, without the written permission of Akron Rubber Development Laboratory, Inc. (ARDL). The information contained herein applies to the specific material, products or processes tested or evaluated. No warranty of any kind is herein construed or implied. The liability of ARDL, Inc. shall be limited to the amount of consideration paid for services. ARDL, Inc. is accredited by A2LA for the test methods listed on the attached scope.

April 16, 2018

**SAS Safety Corporation**  
Todd Zuella

Page 1 of 2 – PN 140575

**SUBJECT:** Permeation testing per ASTM D 6978 on sample submitted by the above company.

**RECEIVED:** One black glove type identified as; Raven Powder-Free Nitrile Examination Gloves; 6 mil; Mediums; 66517; Lot# YN735820387.

**TEST DRUG:**

Table 1. List of the Testing Drugs, Sources, and Expiration Dates

TESTING DRUG	DRUG SOURCE
Fentanyl Citrate Injection, 100mcg/2mL	Hospira; Lot# 80-337-DK; Expiration 2/1/2019

**COLLECTION MEDIA:**

The collection media, which were selected, are listed in Table 2.

Table 2. Collection Media for Testing Drugs

TEST DRUG AND CONCENTRATION	COLLECTION MEDIUM
Fentanyl Citrate Injection, 100mcg/2mL	Distilled Water

**TESTING CONDITIONS:**

Standard Test Method Used:	ASTM D 6978
Analytical Method:	UV/VIS Spectrometry
Testing Temperature:	35.0°C ± 2.0
Collection System:	Closed Loop
Specimen Area Exposed:	5.067 cm <sup>2</sup>
Selected Data Points:	25/test
Number of Specimens Tested:	3/test
Location Sampled From:	Cuff area
Deviation from Standard Test Method:	Used 1" Permeation Cell

**DETECTION METHOD OF CHEMICAL PERMEATION; UV/VIS ABSORPTION SPECTROMETRY:**

Instrument: Perkin Elmer UV/VIS Spectrometer Lambda 25

UV/VIS Absorption Spectrometry was used to measure the absorbance of test chemicals, which permeated through the specimens into the collection medium. The collection medium was circulated in a closed loop at 11 ml/minute of flow rate through the testing period. Data collection was performed according to the programmed schedule by means of UV Winlab software from the Perkin Elmer Corporation. The list of the characteristic wavelengths is shown below.

Table 3. Characteristic Wavelengths used in UV/VIS Absorption Spectrometry

TEST DRUG	WAVELENGTH (nm)
Fentanyl Citrate Injection, 100mcg/2mL	199

**SAMPLE CHARACTERISTICS:**

Table 4. Thickness characteristics for the tested specimens: One black glove type identified as: Raven Powder-Free Nitrile Examination Gloves; 6 mil; Mediums; 66517; Lot# YN735820387.

Testing Drug	Thickness (mm)			Average (mm)	Weight/Unit Area (g/m <sup>2</sup> )
	Sample 1	Sample 2	Sample 3		
Fentanyl Citrate	0.098	0.099	0.104	0.100	98.8

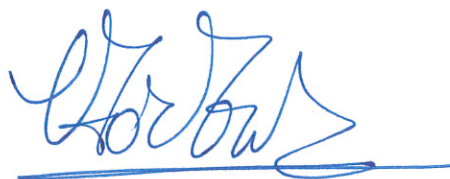
**RESULTS:**

Table 5. Permeation Test Results on: One black glove type identified as: Raven Powder-Free Nitrile Examination Gloves; 6 mil; Mediums; 66517; Lot# YN735820387.

TEST DRUG AND CONCENTRATION	MINIMUM BREAKTHROUGH DETECTION TIME (Specimen 1/2/3) (Minutes)	STEADY STATE PERM. RATE (Specimen 1/2/3) (µg/cm <sup>2</sup> /minute)	OTHER OBSERVATIONS
Fentanyl Citrate Injection, 100mcg/2mL	No Breakthrough up to 240 minutes	N/A	Slight swelling; no degradation



**Tiffany L. Heller**  
Assistant Manager,  
Pharmaceutical Services

**AKRON RUBBER DEVELOPMENT LABORATORY, INC.**

**Ana C. Barbur, M.S.**  
Vice President,  
Analytical & Chemical, Services